


Vortex Flow Meter

User Manual

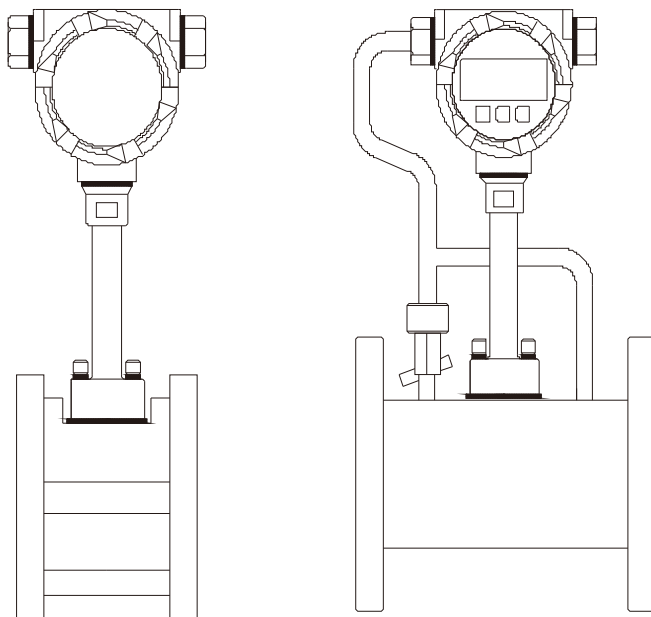

Color is changed without notice.

I . Introduction	3
II . Working Principle	3
III. Technical Parameters.....	4
III. I Physical Parameters.....	4
III. II Electrical parameters.....	13
III. III Menu Display and Parameters setting.....	13
IV. Installation Instruction.....	20
Appendix I : Functions Schedule of all Models	23
Appendix II : Configuration Size of Flange Connection Models	25
Appendix III : Configuration Size of Wafer Connection Models.....	26
Appendix IV: Calibration Method.....	27
Appendix V: Fundamental Formula.....	27
Appendix VI: Communication Function	28
Appendix VII: Electrical Wiring.....	30

I. Vortex Flowmeter Instruction


Vortex Flowmeter is on the principle of Karman street, to measure liquid, gas and vapour even turbid liquid including micro grain and impurity.

Applications: petroleum, chemical industry, paper making, metallurgy, electric force, environmental protection, food industry and etc.

II. Working Principle

LUGB & LUCB Vortex flowmeter work on the principle of generated vortex and relation between vortex and flow by theory of Karman and Strouhal, which specialize in measurement of steam, gas and liquid of lower viscosity.

As shown in below illustration, medium flows through bluff body and then vortex is generated, vortices are alternately formed on both sides with opposite directions of rotation, Vortices frequency is directly proportional to medium velocity. Through numbers of vortices that is measured by sensor head, medium velocity is calculated, plus flowmeter diameter, final volume flow come out.

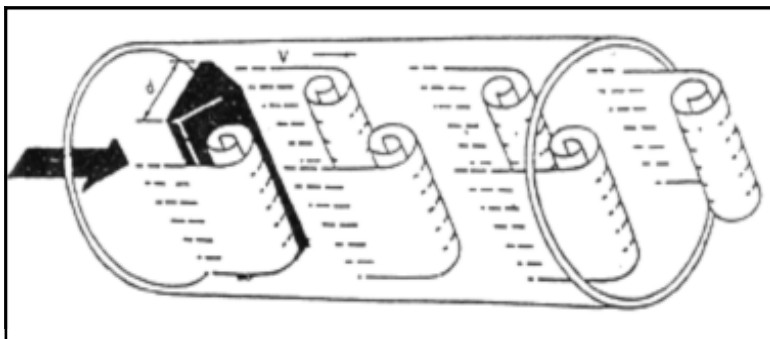

Computational formula as follows:

$F = St \cdot V / md$ Formula 1

$Q = 3600 \cdot F / K$ Formula 2

$M = Q \cdot p$ Formula 3

Among Formula:

- ★ F..... Fluid flow through bluff body generate frequency of vortex (Unit : Hz)
- ★ St... Strouhal constant (zero dimension)
- ★ V..... Mean velocity of fluid inside the pipeline (Unit : m/s)
- ★ m..... The ratio between Lune Circulation area of bluff body at both sides and cross-sectional area (Unit: zero dimension)
- ★ d..... Upstream face width of bluff body inside vortex flowmeter (Unit : m)
- ★ D..... Inside diameter (ID) of vortex flowmeter (Unit : m)
- ★ Q..... Instantaneous volume flow (Unit : m³ / h)
- ★ K..... Instrument coefficient of vortex flowmeter (Unit : pulses / m³)
- ★ M..... Instantaneous mass flow (Unit : kg/ h)
- ★ p..... Fluid density (Unit : kg/ m³)

Note: vortex flowmeter "K" coefficient is corresponding with one diameter, the exact "K" value should be calibrated in practice. Viz. one cubic meter fluid through sensor output numbers of pulse under working condition.

III. Technical Parameters

III. I Physical Parameters

Medium: liquid , gas (including natural gas), steam (saturated steam and superheated steam)

Normal diameter

LUGB Pipeline-version: DN10-DN500 LUCB insertion-version: DN200-DN2000

Accurate:

LUGB Pipeline-version: 1.0% 1.5% (0.2% & 0.5% supply by negotiation) LUCB insertion-version: 2.5% (1.0%&1.5% supply by negotiation)

REFERENCE FLOW RANGE AS PER BELOW DIAGRAMS.

Velocity scope of flow about intelligent digital filtering vortex flowmeter Liquid (0.30 m/s...10 m/s), Gas/steam (3.0 m/s...90 m/s)

Normal pressure:

LUGB pipeline-version wafer connection: DN10-DN500 (priority PN2.5MPa) LUGB pipeline-version flange connection: DN10-DN80 (priority PN2.5MPa) DN100-DN200 (priority PN1.6MPa) DN250-DN500 (priority PN1.0MPa) LUCB insertion-version attachment flange: DN200-DN2000 (priority PN1.6MPa)

Note : wafer-version vortex flowmeter assemble made-to-order flanges, when flowmeter leave factory including companion flanges. We are able to provide GB/T9119-2000, ANSI/ASME, DIN, JIS, KS.... Standard flanges (GB-China standard priority), pressure class recommend priority level.

Medium temperature

LUGB pipeline-version: $-40^{\circ}\text{C} \sim +160^{\circ}\text{C}$ $-40^{\circ}\text{C} \sim +280^{\circ}\text{C}$ - $40^{\circ}\text{C} \sim +350^{\circ}\text{C}$ - $40^{\circ}\text{C} \sim +420^{\circ}\text{C}$

LUCB insertion-version: $-40^{\circ}\text{C} \sim +160^{\circ}\text{C}$ $-40^{\circ}\text{C} \sim +200^{\circ}\text{C}$

Ambient conditions:

Ambient temperature: $-20^{\circ}\text{C} \sim +60^{\circ}\text{C}$ (normal); $-20^{\circ}\text{C} \sim +40^{\circ}\text{C}$ (explosion-proof) Relative humidity (RH): 5% - 95%RH

Atmospheric Pressure: 86kPa - 106kPa

Electrical Interface: M20*1.5 internal thread (priority). Protection level : IP65 (IP67, IP68 supply by negotiation)

Explosion-proof class: Intrinsic safety Exia II CT4; Exib II CT4; Flame-proof Exd II CT6

Main body material: stainless steel (other material supply by negotiation) Pressure lose: $\Delta P \leq 1.2 P_s$ V2 (ΔP unit is Pa, P_s unit is kg/m³, V unit is m/s)

Calibration method : all flowmeters should be calibrated in the way of lower reaches taking pressure before flowmeters leave factory.

III. I . I

LUGB and LUCB Vortex Flowmeter configuration & size


LUGB wafer connection vortex flowmeter: special companion flanges.

LUGB flange connection vortex flowmeter: see appendix 3 & 4 flanges size of configuration. we are able to provide GB (China); ANSI; DIN; JIS and etc.


LUCB insertion-version vortex flowmeter: flanges choose DN100 standard flange

Dimensions of vortex flowmeter as per fig2 and fig1


1. Wafer connection

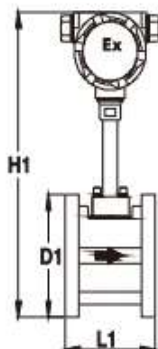

2. Flange type

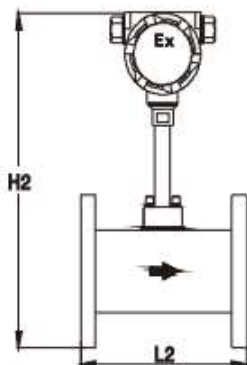

3. Flange type with temperature and pressure compensation

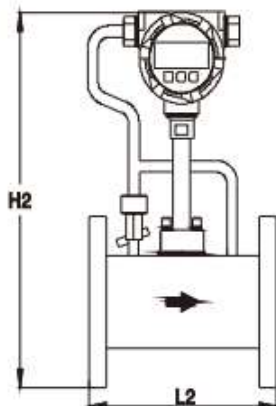

LUGB and LUCB vortex flowmeter max configuration size fig. 1 (unit: mm)

Items	H1 ^a	H1 ^b	H1 ^c	D1	L1	H2 ^a	H2 ^b	H2 ^c	L2
DN15	525	445	355	45	65	540	460	370	170
DN20	531	451	361	58	65	545	465	375	170
DN25	531	451	361	58	65	550	470	380	250
DN32	531	451	361	58	65	563	483	393	250
DN40	529	449	359	85	70	578	498	408	250
DN50	541	461	371	99	70	590	510	420	250
DN65	558	478	388	118	70	612	532	442	250
DN80	573	493	403	132	70	625	545	455	280
DN100	595	515	425	156	70	644	564	474	300
DN125	621	541	451	184	70	674	594	504	350
DN150	647	567	477	211	70	703	623	533	350
DN200	705	625	535	266	98	757	677	587	400
DN250	757	677	587	319	114	810	730	640	450
Dn300	808	728	638	370	130	860	780	690	500

P.LUCB Insertion-Vortex Flowmeter 's Connection

between amplifier and sensor

1.stop medium flow to dismantle

2.keep medium flow to dismantle

Q.The mode of wave filtering

1.common mode

2.Intelligent Digital filtering mode

R.LUCB Insertion-version Vortex flanges
pressure class

1.PN1.6Mpa (priority)

2.PN2.5MPa (pressure class >2.5 MPa supply
by negotiation)

Attention: integrated P/T compensation Compact vortex apply in steam measurement, if designing drainage receiver configuration. Then Horizontal Installation is required. If vertical installation or leaning installation condensing drainage loop receiver is required.

Notes : each functions see appendix one.

III. I . II

LUGB pipeline-version vortex flowmeter measurable flow range (refer to Fig2~5)

Notes : when choose vortex flowmeter that keep medium flow with dismountable sensor head or vortex flowmeter with accuracy is $\pm 0.5\%$, the lower limit of flow range is 1.5 times of corresponding value from fig 2~4, upper limit multiplied by 0.8

LUGB vortex flowmeter measurable liquid of different density corresponding with flow range under working condition fig. 2

Liquid flow range											
Density (kg/m ³)	500	600	700	800	900	1000	1200	1400	1600	1800	Qmax
DW	Different density liquid, the mini flow rate Qmin(Unit:m ³ /h)										□Unit:m ³ /h)
DN15	0.66	0.55	0.52	0.41	0.4	0.39	0.33	0.31	0.29	0.26	4.5
DN20	1.27	1.1	1.08	0.99	0.88	0.66	0.64	0.62	0.59	0.57	8
DN25	1.43	1.32	1.21	1.16	1.1	0.99	0.9	0.84	0.78	0.75	12
DN32	2.09	1.98	1.87	1.78	1.72	1.65	1.6	1.49	1.32	1.1	20
DN40	3.85	3.52	3.3	3.08	2.86	2.51	2.42	2.31	2.2	2.09	32
DN50	5.17	4.73	4.29	4.07	3.96	3.85	3.3	3.08	2.86	2.75	50
DN65	7.81	7.15	6.93	6.82	6.71	6.6	5.5	4.95	4.62	4.4	84
DN80	12.1	11	10.56	10.12	10.01	9.9	8.8	8.36	7.7	6.6	127
DN100	22	19.8	18.7	17.6	16.5	15.4	14.3	13.2	11	9.9	198
DN125	30.8	28.6	27.5	26.4	25.3	24.2	23.1	22	19.8	15.4	310
DN150	57.2	55	49.5	46.2	39.6	35.2	33	30.8	28.6	22	445
DN200	108.9	96.8	85.8	77	68.2	62.7	58.3	55	47.3	38.5	791
DN250	202.4	181.5	165	143	121	97.9	88	79.2	74.8	60.5	1237
DN300	275	242	220	198	176	140.8	132	121	107.8	84.7	1780

LUGB Vortex flowmeter measure gas of different density corresponding with flow range under standard condition fig.3

gas flow range													
Density (kg/m ³)	0.5	0.8	1.2	2.4	3.6	4.8	6	7.2	8.4	9.6	12	20	Qmax
DW	Different density liquid, the mini flow rate Qmin(Unit:m ³ /h)												(Unit: m ³ /h)
Dn15	5.28	3.85	3.52	3.08	2.97	2.86	2.75	2.64	2.53	2.42	2.31	2.2	38
DN20	9.02	7.26	5.5	5.28	5.17	4.95	4.73	4.4	4.29	4.18	4.07	3.3	67
DN25	11	9.9	8.69	8.36	7.92	7.59	7.26	6.82	6.49	5.94	5.5	4.95	100
DN32	28.6	19.8	15.4	14.52	14.08	13.42	13.2	12.87	12.32	11.99	11.11	9.9	170
DN40	41.8	27.5	22	20.9	19.8	18.7	17.6	16.5	15.4	14.3	13.2	11	300
DN50	52.8	44	34.1	31.9	30.8	28.6	25.3	24.2	23.1	22	19.8	13.2	500
DN65	88	72.6	58.3	49.5	48.4	46.2	44	41.8	38.5	33	28.6	19.8	780
DN80	143	110	88	83.6	77	72.6	68.2	63.8	55	50.6	41.8	30.8	1200
DN100	198	176	132	121	110	99	88	77	68.2	61.6	52.8	38.5	2000
DN125	308	275	209	187	171.6	159.5	148.5	132	110	99	83.6	60.5	2900
DN150	418	341	308	286	264	242	220	198	176	154	121	93.5	4100
DN200	880	660	550	528	473	440	418	396	363	330	297	220	7500
DN250	1100	968	869	803	748	682	649	572	528	462	440	330	12500
Dn300	1430	1309	1254	1166	1078	990	902	836	770	682	638	440	16500

Conversion formula of gas volume flow under working condition & volume flow under standard condition:

$$Q(\text{Ambient}) = Q(\text{Standard}) * P(\text{Standard}) * Z * (273.15 + T(\text{Ambient})) / [(P(\text{Ambient}) + P(\text{Ambient})) * (273.15 + T(\text{Standard}))] \text{--- FORMULA 4}$$

Among formula :

Q (Ambient) --- volume flow under working condition (unit: m³/h)

P (Ambient) --- gas pressure under working condition (unit: Mpa)

T (Ambient) --- gas temperature under working condition (unit: ℃)

Z ----- gas relative compressibility $Z = Z_s / Z_N$ (zero dimension)

Q (Standard) --- volume flow under standard condition (unit: m³/h)

P (Standard) --- Atm press under standard condition (take absolute pressure = 0.101325 MPa)

T (Standard) --- temperature under standard condition (0℃ or 20℃)

P (Local) -- local Atm press (unit: Mpa)

LUGB Vortex flowmeter measure saturated steam of different density corresponding with flow range under working condition fig.4

Mpa	0.1	0.2	0.3	0.4	0.5	0.6	0.8	0.9	1	1.2	1.6	2	Unit	
°C	120	134	144	152	159	165	175	180	184	192	204	215		
Kg/m³	1.12	1.67	2.19	2.68	3.18	3.67	4.62	5.16	5.63	6.67	8.52	10.57		
DW	Range	Different steam density corresponding with flow range												
mm														
15	Qmin	3.85	5.67	7.41	9.12	11	12.54	15.95	17.93	19.36	22.55	29.37	36.19	kg/h
	Qmax	35	51.5	67.4	83	100	115	146	163	176	205	268	329	
20	Qmin	6.84	10.07	13.09	16.17	19.58	22.44	28.49	32.01	34.43	40.04	52.25	64.35	
	Qmax	62.2	91.6	120	147	178	204	259	291	313	365	476	586	
25	Qmin	10.68	15.73	20.46	25.3	30.69	34.98	44.55	49.94	53.79	62.59	81.73	100.54	
	Qmax	97.1	143	187	230	279	318	405	454	489	569	743	914	
32	Qmin	17.49	25.63	33.66	41.47	50.27	57.42	72.93	81.95	88.11	102.63	133.1	163.9	
	Qmax	159	234	306	378	457	522	664	745	802	933	1218	1499	
40	Qmin	25.3	36.3	47.3	58.3	70.4	80.3	102.3	110	121	143	187	231	
	Qmax	300	440	575	710	860	980	1250	1400	1500	1750	2280	2810	
50	Qmin	38.5	38.5	57.2	69.3	83.6	96.8	122.1	137.5	143	165	220	275	
	Qmax	550	460	680	845	1020	1170	1480	1670	1800	2100	2730	3360	
65	Qmin	64.9	95.7	125.4	150.7	182.6	209	264	303.6	326.7	379.5	495	605	
	Qmax	790	1160	1520	1835	2222	2540	3230	3620	3970	4620	6030	7422	
80	Qmin	98.45	144.1	189.2	233.2	282.7	319	407	451	495	572	748	924	
	Qmax	1195	1760	2300	2800	3400	3900	4900	5580	6000	6999	9100	11000	
100	Qmin	0.15	0.22	0.3	0.36	0.44	0.51	0.64	0.72	0.77	0.9	1.1	1.43	t/h
	Qmax	1.87	2.75	3.6	4.43	5.36	6.12	7.78	8.73	9.4	11	14.3	17.6	
125	Qmin	0.24	0.35	0.46	0.56	0.68	0.78	1	1.1	1.21	1.41	1.84	2.2	
	Qmax	2.91	4.29	5.62	6.91	8.37	9.56	12	13.6	14.7	17	22.3	27.4	
150	Qmin	0.35	0.51	0.66	0.81	0.99	1.13	1.44	1.62	1.74	2.02	2.64	3.26	
	Qmax	4.2	6.18	8.09	9.96	12	13.8	17.5	19.6	21.1	24.6	32.1	39.5	
200	Qmin	0.62	0.9	1.19	1.45	1.76	2.01	2.56	2.87	3.09	3.61	4.71	5.8	
	Qmax	7.5	11	14.4	17.7	21.4	24.5	31.1	35	37.6	43.7	57.1	70.3	
250	Qmin	0.96	1.41	1.85	2.2	2.76	3.16	4	4.5	4.84	5.61	7.36	9.02	
	Qmax	11.6	17	22	27.6	33	38	48	54	58.7	68	89	110	
300	Qmin	1.38	2.04	2.66	3.28	3.97	4.54	5.78	6.48	6.97	8.12	10.56	12.98	
	Qmax	16.7	24.7	32	39	48	55	70	78	84	98	128	158	

Superheated Steam fig.5 (unit : kg/m³)

ITEM	130°C	140°C	150°C	160°C	170°C	180°C	190°C	210°C	220°C	250°C	300°C	360°C	420°C
0.10MPa	1.1	1.07	1.04	1.02	0.99	0.97	0.95	0.91	0.89	0.83	0.76	0.69	0.63
0.15MPa	1.38	1.34	1.34	1.28	1.24	1.21	1.19	1.13	1.11	1.04	0.95	0.86	0.78
0.26MPa		1.96	1.9	1.85	1.81	1.76	1.72	1.64	1.61	1.51	1.37	1.24	1.13
0.30MPa			2.12	2.067	2.01	1.96	1.92	1.83	1.79	1.68	1.53	1.38	1.26
0.36MPa			2.46	2.39	2.33	2.27	2.21	2.11	2.06	1.94	1.76	1.59	1.45
0.40MPa				2.61	2.54	2.47	2.41	2.3	2.25	2.11	1.91	1.73	1.57
0.50MPa				3.16	3.07	2.99	2.91	2.77	2.71	2.54	2.3	2.07	1.89
0.60MPa					3.61	3.51	3.42	3.25	3.18	2.97	2.69	2.42	2.21
0.70MPa						4.05	3.94	3.74	3.65	3.41	3.09	2.78	2.53
0.80MPa						4.59	4.46	4.23	4.13	3.85	3.48	3.13	2.84
0.90MPa						5.15	4.99	4.73	4.61	4.3	3.88	3.48	3.16
1.00MPa							5.54	5.23	5.09	4.75	4.28	3.84	3.48
1.15MPa							6.37	6	5.84	5.43	4.88	4.37	3.97
1.50MPa								7.87	7.64	7.05	6.3	5.63	5.1
1.65MPa								8.7	8.43	7.76	6.92	6.17	5.59
1.80MPa								9.55	9.24	8.48	7.55	6.72	6.08
2.00MPa									10.36	9.47	8.39	7.45	6.74
2.20MPa									11.51	10.47	9.24	8.2	7.4
2.50MPa										12.02	10.55	9.32	8.39

Several normal gas of density under standard conditionfig. 6 (unit : kg/m³)

Tag	Air	Hydrogen	Oxygen	Nitrogen	Chlorine	Ammonia gas	Semi- watergas
Density	1.293	0.0889	1.43	1.251	3.214	0.77	0.836
Tag	Argon	Acetylene	Methane	Ethane	Propane	Butane	Coke-oven gas
Density	1.79	1.017	0.717	1.357	2.005	2.703	0.4849
Tag	Ethylene	Propylene	Natural gas	Coal gas	CO	CO2	
Density	1.264	1.914	0.828	0.802	1.25	1.977	

Notes: standard state is absolute pressure 0.101325MPa and temperature 0°C.

LUCB insertion-version vortex flowmeter measurable flow range under working condition and its calculation. See fig. 7

LUCB insertion-version vortex flowmeter measure liquid of different density corresponding with flow range under working condition. Fig.7

Gas	Density $\rho(\text{kg/m}^3)$	1	1.2	2	3	4	6	8	10	15	20	Vmax(m/s)
	Vmin(m/s)	5.5	5.2	5	4.8	4.6	4.2	4	3.8	3.6	3.5	55
Liquid	Density $\rho(\text{kg/m}^3)$	500	600	700	800	900	1000	1200	1400	1600	1800	Vmax(m/s)
	Vmin(m/s)	0.96	0.8	0.7	0.66	0.62	0.6	0.56	0.52	0.5	0.45	6

Notes : fig.7 that is accuracy $\pm 2.5\%$ of insertion-version vortex flowmeter flow range. When accuracy is better than $\pm 2.5\%$, velocity of flow = lower limit of velocity multiplied by coefficient $R(R=2-3)$, the upper limit multiplied by 0.8.

LUCB insertion-version vortex flowmeter measurable medium flow range calculation under working condition.

Gas & liquid : min volume flow formula under working condition $Q_{\min}=3600 \cdot V_{\min} \cdot (\pi \cdot D^2/4)$ ----- Formula 5

Gas & liquid : max volume flow formula under working condition $Q_{\max}=3600 \cdot V_{\max} \cdot (\pi \cdot D^2/4)$ -----Formula 6

Gas : min volume flow formula under standard condition

$Q_{N\min}=Q_{\min} \cdot [(\rho_{\text{local}}+\rho_{\text{ambient}}) \cdot (273.15+T_{\text{standard}})]/$

$[P_{\text{standard}} \cdot Z \cdot (273.15+T_{\text{ambient}})]$ ----Formula 7

Gas : max volume flow formula under standard condition

$Q_{N\max}=Q_{\max} \cdot [(\rho_{\text{local}}+\rho_{\text{ambient}}) \cdot (273.15+T_{\text{standard}})]/ [P$

$_{\text{standard}} \cdot Z \cdot (273.15+T_{\text{ambient}})]$ ----- Formula 8 Gas : density formula under working condition

$\rho = \rho_n [(\rho_{\text{local}}+\rho_{\text{ambient}}) \cdot (273.15+T_{\text{standard}})]/ [P_{\text{standard}} \cdot Z \cdot (273.15+T_{\text{ambient}})]$ ----- Formula 9

Among (insertion-version vortex flowmeter) :

$Q_{\min}$ -- min volume flow under working condition (unit : m³/h) $Q_{\max}$ -- max volume flow under working condition (unit : m³/h)

$V_{\min}$ -- min velocity under working condition (unit : m/s refer to fig.7) $V_{\max}$ -- max velocity under working condition (unit : m/s refer to fig.7) D ----- nominal diameter of insertion-version vortex flowmeter (unit : m) π ----- circumference ratio 3.1415926535898

$Q_{N\min}$ - gas min volume flow under standard condition (unit : m³/h)

$Q_{N\max}$ - gas max volume flow under standard condition (unit : m³/h)

T_{standard} ---- temperature under standard condition, general is 0°C or 20°C. (unit:°C)

T_{ambient} ---- measurable gas temperature under working condition (unit:°C) P

$_{\text{standard}}$ ---- normal atmospheric pressure (=0.101325MPa)

P_{ambient} ---- measurable gas pressure under working condition (unit : Mpa)

Z ----- measurable fluid relative compressibility $Z=Z_{\text{ambient}}/Z_{\text{standard}}$

ρ ----- gas density under working condition (unit : kg/m³)

ρ_n ---- gas density under standard state (unit: kg/m³ ; temp is 0°C or 20°C, absolute pressure is 0.101325MPa , among formula 9 the temperature is the same between T_{standard} and ρ_n corresponding

temp. Several normal gas density under standard state see fig. 6) P_{local} --local atmospheric pressure (unit : Mpa)

LUCB insertion-version vortex flowmeter Numerical Methods of flow range matching steam measurement:

According to steam temperature and pressure refer to fig.4 & fig.5 then gain exact density " ρ " **under working condition.**

According to steam density " ρ " under working condition, refer to fig.7 then gain max/min velocity of flow under working condition " V_{max}/V_{min} " .

According to pipe diameter of insertion-version vortex flowmeter, through Formula 5 and Formula 6 calculate min volume under working condition or max volume.

The final density " ρ " under working condition $\times Q_{min} \text{ or } Q_{max} = \text{mass flow range}$.

III. II Electrical Parameter Signal output :

1. Instantaneous flow under working condition corresponding voltage-frequency-pulse output (lower PWL $\leq 1V$, higher PWL $\geq 6V$)
2. Instantaneous flow under standard condition corresponding voltage-frequency-pulse output (lower PWL $\leq 1V$, higher PWL $\geq 6V$)
3. Instantaneous flow under standard condition pulse equivalent output (lower PWL $\leq 1V$, higher PWL $\geq 6V$)
4. Instantaneous flow under working condition corresponding two-wire or three-wire 4~20mA output
(load resistance $\leq 300 \Omega$)
5. Instantaneous flow under standard condition corresponding two-wire or three-wire 4~20mA output (load resistance $\leq 300 \Omega$)

Communication interface: RS485 ; HART Display mode:

A . Intelligent numeric alphabetic display type: twin-row numeric alphabetic LCD (instantaneous flow rate and totalizer)

Intelligent dot matrix LCD: English 128*64 dot matrix LCD(



instantaneous flow rate,

totalizer, temperature and pressure under working condition, battery voltage or density under working condition,


instantaneous flow rate under working condition, send-out, time, menu modify records, power-off records, etc.)

III.III.I. Menu Display

Turn on power 24VDC, the main menu will display. The main menu has 5 sub-page, which can be displayed & switched by the **button (K2)**.

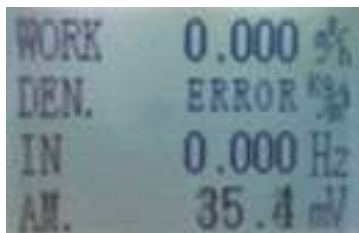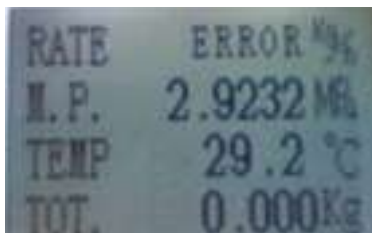

Connect the hand operator to the flow meter, and press the button(K1) for several second, then the hand operator starts receiving the data and displaying the main menu.



Menu instruction

Instantaneous flow: display range 0.000-99999999

Total flow: display

Range 0.000-999999999

Remarks: When the total flow is accumulated to 1000000000, it is all cleared and re-accumulated. When the flow unit changes, the total flow value remains at the original value. In this case, please record down the original total flow, then clear it and re-accumulate.

Temperature: display range -50.0...430.0

Gauge pressure/Absolute pressure -0.1000...20.0000MPa

When the unit is MPa, range is -0.1000...20.0000MPa;

Working condition: Display instantaneous volume flow under working condition, range is 0.000-99999999m³/h

Density: 0.000-99999999kg/m³

K-factor: When choose Nm³/h (standard condition), the compression factor will display with medium under working condition, range is 0.000000-9.999999

Input: The frequency value that actually measured by the sensor, range is 0.000-9000.0Hz Output: Display the corresponding frequency or current output value according to the "output type" setting in the menu

Instrument Temperature: Display inside temperature of amplifier, range is -99.9-+99.9

Upper-limit: when the measurement limitation function open, transmitter will show the cumulative flow over the upper limit, range is 0.000-999999999

Noted: When the upper-limit flow rate up to 1000000000, all the record will be reset and reaccumulate.

Parameter set: Times of parameters setting, range is 0-9999, if up to 10000 times, the value will be re-set.

Menu four: Display current time, total power fail minutes; "system time" will be shown when flow meter turn on

Menu five: Display the power failure record, will save the last 10 times of power failure; "DATE" will be shown when flow meter turn on special display instructions

NULL: No display

B.ERROR: Data errors, check parameter setting or flow meter operation

C.OVERRUN: Data beyond display range

III.III.II. Parameter Setting

Parameters could be set by  button(K1),  button(K2),  button(K3),  button(K4)

1. Button function

K1 button: enter parameter setting and setting confirmation

K2 button: Move the cursor to the next position

K3 button: Increase value or function selection

K4 button: return to last menu

Parameter setting

Validation setting

Language

2. Main menu

Press K1 to enter main menu

Press K2 to select each menu, press K1 to enter

3. Main menu of parameters setting

	input password
Parameter setting	000000
Totalizer flow reset	123000
Flow zero setting	000000
Password setting	000000

After selecting menu, press K1 to enter password menu, input password; then set each parameter.

Noted: If there is no operating in the parameter setting menu over 30 seconds, the system will automatically exit the “Settings” state. Meanwhile, the setting parameter value is invalid. All the parameters setting will be workable by storage confirmation before exiting

3. 1 Parameters Setting Menu

Initial password: 000000

Parameters Setting Menu (table one)

Menu	Menu Content	Explanation
LOAD DEFAULT	YES or NO	Select "YES", press the setting button until the LCD displays "Please wait...", then will display "Restore completed"; select "NO", to enter the next menu. Default setting is display "NO".
APPLICATION	LIQUID GAS GAS+P+T HEAT STEAM+P+T SAT. STEAM+T SAT. STEAM+P WATER +P+T LIQUID COMP. OIL+P+T NATURAL GAS +P+T MIXED GAS+P+T	
SIZE	0000- 9999mm	
FACTOR UNIT	1/m3、1/L	
K-FACTOR	K-FACTOR LINEAR FLOW CURVE K-FACTOR	K-factor setting range: 0.000000-99999999 Linear frequency modification setting range: 0.00-9999Hz Method of linear correction settings please kindly check chapter 6
	FLOW CURVE	
	POINT 1 K 1 POINT 2 K 2 POINT 10 K 10	
FLOW UNIT	m3/h、 km3/h、 l/min、 kg/h、 t/h、 kg/min、 (Nm3/h、 Nkm3/h、 NI/min、 Nm3/min、 Nkm3/min)	m3/h; km3/h; l/min are the volume flow unit under the working condition; kg/h; t/h; kg/min are mass flow unit; Nm3/h; Nkm3/h; NI/min; Nm3/min; Nkm3/min are gas volume flow unit

OUTPUT	UNSCALE PULS (calibration) COMP. PULSE 4-20mA	UNSCALE PULSE: only output the frequency pulse before compensation COMP. PULSE: Output the frequency after correction and compensation 4-20mA: Display and output the 4-20ma current at the upper and lower limit of output
SCALED FACTOR	0.000000-99999999	The scaled factor is only workable when output type is "COMP. PULSE". Scaled factor should be selected according to the flow rate. For calculation formula, please refer to appendix 3.
HIGH FLOW	0.000000-99999999	It's workable under "4-20mA" output
LOW FLOW	0.000000-99999999	
DAMPING	00-99	"LIQUID COMP." parameter setting
TEMP. 1	- 9999~99999℃	
FLUID DENSITY 1	0.000000-99999999kg/m3	
TEMP. 2	- 9999~99999℃	
FLUID DENSITY 2	0.000000-99999999kg/m3	
TEMP. 10	- 9999~99999℃	
FLUID DENSITY 10	0.000000-99999999 kg/m3	
CO2 MOLE FRACTION	0.000000-99999999	Parameter setting for "NATURAL GAS +P+T" "CO2 MOLE FRACTION" default value 0.006; "H2MOLE FRACTION" default value 0; "RELATIVE DENSITY" default value 0.581 "QGR" default value 40.66MJ/m3
H2 MOLE FRACTION	0.000000-99999999	
RELATIVE DENSITY	0.000000-99999999	
QGR	0.000000-99999999MJ/m3	
COMPENSATION OF COMP. FACTOR	AUTO, MENU	

COMP. FACTOR	0.000000-99 999999	"COMPENSATION OF COMP. FACTOR" is available when choose "MENU"
CRITICAL PRES	0.000000- 99999999MPa	'GAS +P +T" and "MIXED GAS +P +T" parameter setting.
CRITICAL TEMP	0.000000- 99999999K	"COMPENSATION OF COMP. FACTOR" is available when choose "AUTO"
GAS PRESSURE	0.000000-99999999MPa	Default value: 0.101325Mpa
STD.TEMP. °C	00-99	Default value: 0 °C
COMPENSATION OF T	AUTO, MENU	
TEMP. DATA SET	-50-430 °C	Temperature compensation model is workable when choose "MENU".
PRES UNIT	MPa 、 KPA 、 BAR	
COMPENSATION OF P	AUTO, MENU	
M.P. DATA SET	-0.1-+20MPa	Pressure compensation model is workable when choose "MENU".
FLUID DENSITY 99999999KG/M3	0.000000	No compensation model: The density should be under working condition: Gas temperature compensation: The density should be under 0.101325Mpa and standard temp. Petroleum temperature compensation: The density should be under 0.101325Mpa and 20 °C woodworking tem
FLOW CUTOFF UNIT Hz	Hz, UNIT	
CUTOFF DATA	0.000000-99999999	
DATE	NO, YES	
TIME SETTING	00 YY 00 MM 00 DD 00 HH 00 MM	The time will not display when choose "NO".
COMMUNICATION	NO 485	
DDRESS	001-255	Default: 001
BAUDRATE	9600; 4800; 2400; 1200	Default: 9600

★ 2. When enter menu, some value maybe different with original value. The reason comes from non-flushed LCD screen, it's normal. You could press K2 to recover.

3.2 Total flow reset

★Notice: Non-professional people are forbidden to change the Zero point manually.

★Auto Zero setting

★1. One Key zero setting: On the main interface, press(K3) until the light is on to enter the auto setting status. When the light off, the setting is finished.

★2. Two key zero setting: Enter the auto setting status first. When the value becomes stable, press (K1), and save setting.

Notice: When setting zero point, please make sure the flow is zero in the pipe.

IV. Installation Instruction

Installation Place and Environment Selection

Try to avoid strong power equipment, high-frequency equipment and strong power switchgear.

Try to avoid high-temp thermal source and source of radiant heating; outdoor installation should do some measures of sun-shading and rain shelter.

Try to avoid shock places and corrosion environment ; meanwhile, easy maintenance should be considered. Reasonable and correct installation position. Installation position should avoid strong shock pipeline, or take some measures of shock absorption. Horizontal, vertical and slanting installation. Liquid measuring ensure flow direction from low to high. Gas measuring, direction no required.


When measuring vapor or high-temp gas, flow meter body pillar should be at an angle of 45 Deg with vertical direction.


Grounding requirement.

When pipelines without available grounding conditions, a ground-wire is essential between housing and earth. Straight length requirement

In order to correct measurement, upstream or downstream of flow meter should obligate enough straight length. No components to effect fluid velocity in upstream of flow meter. All types of straight length installation reference:

LUGB Vortex Flowmeter Straight Length Size Drafts

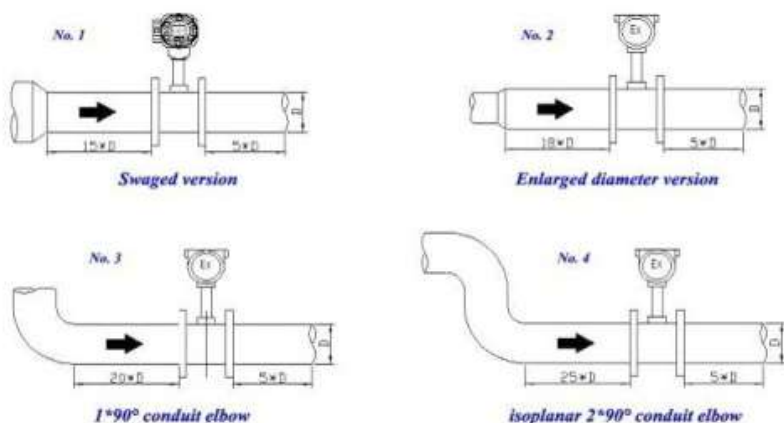

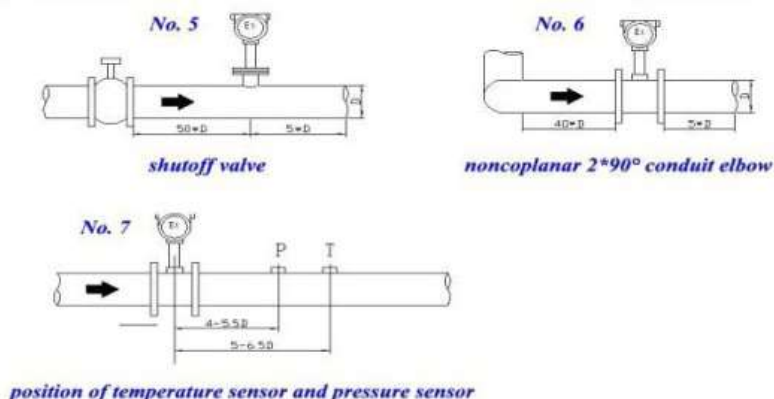



Installation and welding of flow meter

LUGB Vortex diameter is accordant to upstream and downstream tubing diameter at installation point; sensor is concentric with pipeline; prohibit gaskets between sensor and flanges bulge out into pipeline. Make sure that the connection end face of insertion-version vortex flowmeter parallel to the pipe axis. Details as per fig.4.

After initial installation, when medium is steam or other high-temp medium, flanges & bolts should be re-tightened when medium full of pipeline. Do heat reservation measures for pipeline in order to protect amplifier.

LUGB Vortex installation & Welding Reference Figure

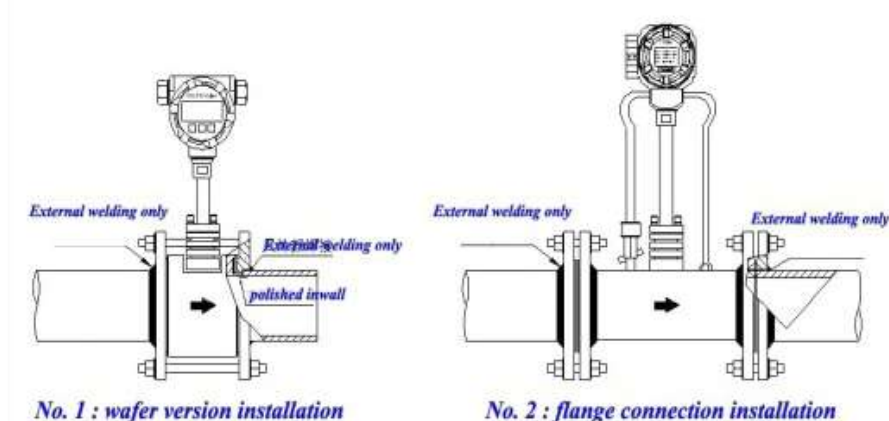

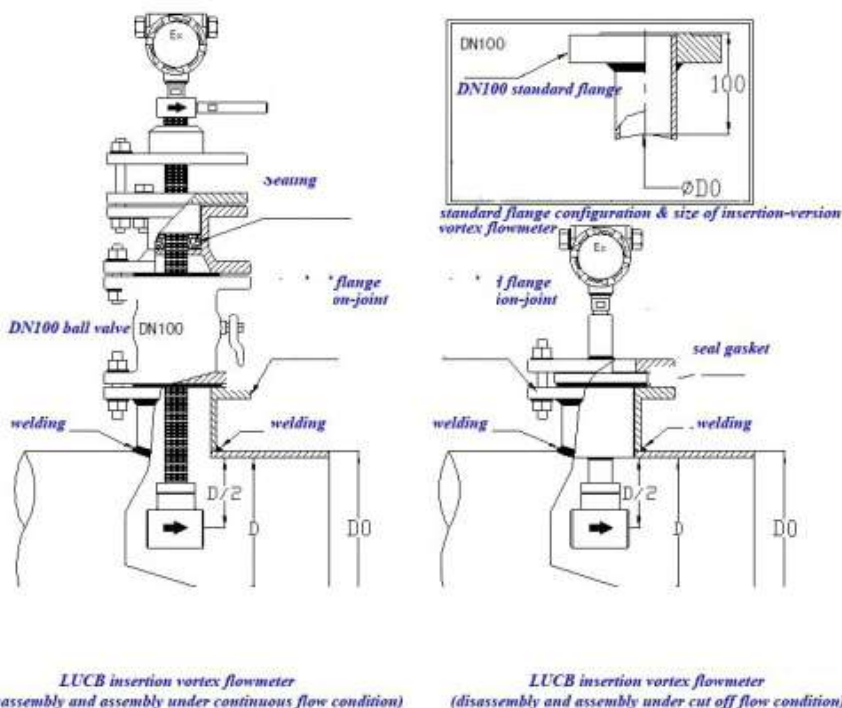


Be attention: concerning P/T compensation integrated vortex flow meter, to avoid high-temp or liner shock damage pressure transmitter, Pressure control valve must be closed before medium is full of pipeline. When medium full of pipeline meanwhile approaching working temperature and pressure, slowly turn on control

valve. Pressure tapping and pressure detector should be done heat reservation if flow meter outdoor installation.

Tag	DN	Medium	Medium temp	Function description
Wafer Connection	Dn10-500 (mm)		-40...+150 °C	Flowmeter body material: stainless steel Wafer type companion flange: forged carbon steel Max working pressure: 2.5Mpa (over 2.5Mpa supply by negotiation)
Flange Connection			-40...+280 °C	
Wafer connection Patent type	DN25-500 (mm)	Gas Liquid Saturated steam Superheated steam	-40...+350 °C	Flowmeter body material: stainless steel (other material supply by negotiation) Max working pressure: 2.5Mpa (over 2.5Mpa supply by negotiation) Features : replace sensor head without effect fluid flow inside pipeline.
Flange connection Patent type			-40...+150 °C	
Flange connection Low flow version equipped dismountable sensor head			-40...+280 °C	Flowmeter body material: stainless steel (other material supply by negotiation) Max working pressure: 2.5Mpa (over 2.5Mpa supply by negotiation) Features : 1.Compare same diameter vortex flowmeter its more lower limit. Replace sensor head without effect fluid flow inside pipeline.
Flange connection Low flow version			-40...+350 °C	
Flange connection Low flow version			-40...+420 °C	
Wafer version with temp compensation	Dn25-500 (mm)	Saturated steam	+100...+220 °C	Flowmeter body material: stainless steel (other material supply by negotiation) Flanges material: forged carbon steel Temperature gauge head: PT100 Max working pressure : 2.5Mpa Features : 1.Special for saturated steam. Integrated flow and temperature sensor in one. 2.Sensor is dismountable type, replace sensor head without effect fluid flow inside pipeline.
Wafer version with Temperature Compensation equipped dismountable sensor head				

Flange connection Integrated temperature with pressure compensation	DN25-500 (mm)	Gas Saturated steam Superheated steam	40...+150 °C	Flowmeter body material: stainless steel (other material supply by negotiation) Temperature gauge head: Pt100 Pressure gauge head: diffuse silicon pressure sensor. Max working pressure: 2.5Mpa (over 2.5Mpa supply by negotiation) Features : 1.Integrated temperature and pressure compensation in one. 2.Sensor is dismountable type, replace sensor head without effect fluid flow inside pipeline.
			-40...+28 °C 0 °C -40...+35 °C 0 °C	
Flange connection Integrated temperature with pressure compensation equipped dismountable Sensor head			-40...+15 °C -40...+28 °C -40...+35 °C 0 °C -40...+42 °C 0 °C	
Insertion-version with dismountable body need stop medium flow	DN200-2000 (mm)	Gas Liquid Saturated steam Superheated steam	-40...+160 °C	Flowmeter body material: stainless steel Connection joint: carbon steel Max working pressure: 2.5Mpa (over 2.5Mpa supply by negotiation) Features: 1.Stop medium flow is the priority for insertion vortex flowmeter. Its compact conformation and good anti-vibration performance. No need stop medium flow with dismountable flowmeter body is equipped DN100 glove valve. Do installation, maintenance and replacement without effect medium flow.
Insertion-version with dismountable body no need stop medium flow			-40...+200 °C	
Submergible-version vortex flow meter	Wafer-version	Gas Liquid	-40...+150 °C -40...+28 °C	Flowmeter body and flange material: same Max working pressure: 2.5Mpa (over 2.5Mpa supply by negotiation) Features : 1.Flowmeter sensor is Submergible-version. Application: subsurface and Submergible pipeline. 2.Remote-version: transmitter and sensor is separated installation. (The biggest distance suggest ≤10m.)
	Flange-version			
	Insertion-version			

Appendix 2: Configuration Size of Flange Connection Models

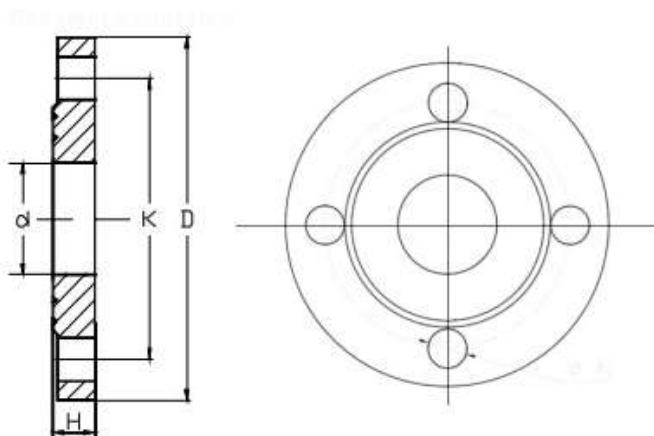


Flange diameter (mm)	Pressure class (MPa)	Flange standard of connection version					
		D(mm)	K(mm)	ε(mm)	N	H(mm)	D(mm)
DN10	PN1.0/PN1.6/PN2.5	90	60	14	4	14	7.2
DN15	PN1.0/PN1.6/PN2.5	95	65	14	4	14	21.3
DN20	PN1.0/PN1.6/PN2.5	105	75	14	4	16	26.9
DN25	PN1.0/PN1.6/PN2.5	115	85	14	4	16	33.7
DN32	PN1.0/PN1.6/PN2.5	140	100	18	4	18	42.4
DN40	PN1.0/PN1.6/PN2.5	150	110	18	4	18	48.3
DN50	PN1.0/PN1.6/PN2.5	165	125	18	4	20	60.3
DN65	PN1.0/PN1.6/PN2.5	185	145	18	4/4/8	20/20/22	76.1
DN80	PN1.0/PN1.6/PN2.5	200	160	18	8	20/20/24	88.9
DN100	PN1.0/PN1.6/PN2.5	220/220/235	180/180/190	18/18/22	8	22/22/26	114.3
DN125	PN1.0/PN1.6/PN2.5	250/250/270	210/210/220	18/18/26	8	22/22/28	139.7
DN150	PN1.0/PN1.6/PN2.5	285/285/300	240/240/250	22/22/26	8	24/24/30	168.3
DN200	PN1.0/PN1.6/PN2.5	340/340/360	295/295/310	22/22/26	8/12/12	24/26/32	219.1
DN250	PN1.0/PN1.6/PN2.5	395/405/425	350/355/370	22/26/30	12/12/12	26/29/35	273
DN300	PN1.0/PN1.6/PN2.5	445/460/485	400/410/430	22/26/30	12/12/16	28/32/38	323.9
DN350	PN1.0/PN1.6/PN2.5	505/520/555	460/470/490	22/26/33	16/16/16	30/35/42	355.6
DN400	PN1.0/PN1.6/PN2.5	565/580/620	515/525/550	26/30/36	16/16/16	32/38/46	406.4
DN450	PN1.0/PN1.6/PN2.5	615/640/670	565/585/600	26/30/36	20/20/20	35/42/50	457
DN500	PN1.0/PN1.6/PN2.5	670/715/730	620/650/660	26/33/36	20/20/20	38/46/56	508

Notes: LUGB flange connection vortex flowmeter its flange pressure class: DN10-DN80 is PN2.5MPa; DN100-DN200 is PN1.6MPa; DN250-DN500 is PN1.0MPa;

if over above pressure class, please mention clearly in purchasing order. GB (China flange standard follows GB9119-2000). International standard, such as ANSI/DIN/JIS... Please customer provide clear model number.

Appendix 3: Configuration Size of Wafer Connection Models

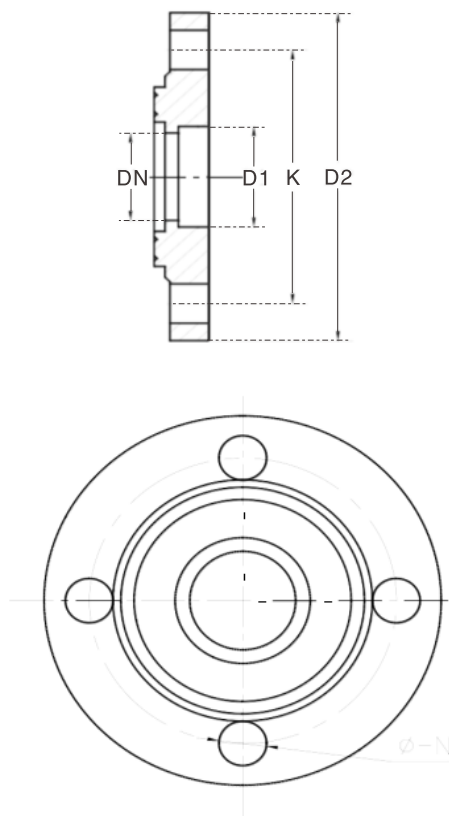

(MPa)	(mm)	flange standard of wafer connection version				
		D1(mm)	D2(mm)	K(mm)	ε(mm)	N(个)
PN1.0/PN1.6/PN2.5	DN10	14	90	60	14	4
PN1.0/PN1.6/PN2.5	DN15	19	95	65	14	4
PN1.0/PN1.6/PN2.5	DN20	26	100	70	14	4
PN1.0/PN1.6/PN2.5	DN25	33	100	75	14	4
PN1.0/PN1.6/PN2.5	DN32	39	105	80	14	4
PN1.0/PN1.6/PN2.5	DN40	49	150	116	18	4
PN1.0/PN1.6/PN2.5	DN50	60	160	124	18	4
PN1.0/PN1.6/PN2.5	DN65	76	175	138	18	4
PN1.0/PN1.6/PN2.5	DN80	90	204	164	20	4
PN1.0/PN1.6/PN2.5	DN100	109	234	192	22	6
PN1.0/PN1.6/PN2.5	DN125	134	250	205	22	6
PN1.0/PN1.6/PN2.5	DN150	163	280	232	22	6
PN1.0/PN1.6/PN2.5	DN200	220	340	286	24	8
PN1.0/PN1.6/PN2.5	DN250	274	390	338	24	8
PN1.0/PN1.6/PN2.5	DN300	327	450	393	26	12
PN1.0/PN1.6/PN2.5	DN350	377	510	460	26	16
PN1.0/PN1.6/PN2.5	DN400	426	565	510	26	16
PN1.0/PN1.6/PN2.5	DN450	482	620	565	30	16
PN1.0/PN1.6/PN2.5	DN500	534	685	620	33	20

Notes: companion flanges for wafer connection follows PN2.5MPa pressure class, when over 2.5MPa please make clearly mention.

Appendix 4: Calibration Method

(1) When calibrating the instrument, the “output form” must be set to “frequency of working condition”, and “value of small signal cutting” is set to 0; after calibration, “K-factor” is set according to the actual calibration, and then change “output form” and “value of small signal cutting” back to the original setting.

(2) Flow rate stabilization time of calibration point: ≥60s

Appendix 5: Fundamental Formula

(1) Instantaneous volume flow rate of working condition

$$Q_v = 3600 \times \frac{F}{K}$$

Q_v - volume flow rate of working condition (Unit: m³/h/ F – current frequency of working condition (Unit: Hz)

K - K factor (Unit: number of pulse/ m³)

(2) Instantaneous mass flow rate of working condition

$$Q_m = 3600 \times \rho \times \frac{F}{K}$$

Q_m—Mass flow rate of working condition (unit: kg/h)

ρ — medium density under working condition (unit: kg/m³)

(3) Scaled coefficient calculated method

$$\begin{cases} K_N = \frac{Q_{max}}{F_N \times 3600} & \text{FLOW UNIT}^*/\text{h} \\ K_N = \frac{Q_{max}}{F_N \times 60} & \text{FLOW UNIT}^*/\text{min} \end{cases}$$

KN – Scaled coefficient (unit: cumulative flow rate / pulse)

FN—Maximum frequency output (unit: Hz; when KN is selected, set FN<5000, and general FN should be 2000Hz)

Q_{max}—the actual maximum instantaneous flow rate (unit: same as the setting flow rate unit)

Appendix 6: Communication Function

(1) Relevant Parameters

The instrument has RS485 communication interface, adopts standard MODBUS-RTU communication protocol, relevant parameters are as follows:

Start bit: 1 bit	Data bit: 8 digits	Parity bit: can be set
Termination bit: can be set	Baud rate: can be set	response time : 0.05s

(2) Data Format

IEEE754 standard single float format

(3) Data Address

This flow meter can transmit 1-16 continuous data at the same time, and each data is stored by the corresponding address as follows:

- 1.0001H: Instantaneous flow value
- 2.0003H: Cumulative flow value
- 3.0005H: Working temperature (Non-compensation model, it displays 0.0000)
- 4.0007H: Gauge Pressure/ absolute pressure (Non-compensation model, it displays 0.0000)
- 5.0009H: Volume flow rate of working condition
- 6.000BH: Density under working condition
- 7.000DH: compression coefficient (Non-standard condition volume unit, it displays 0.0000)
- 8.000FH: Input frequency
- 9.0011H: Frequency output under working condition (Not this output, it displays 0.0000)
- 10.0013H: Scaled pulse output (Not this output, it displays 0.0000)
- 11.0015H: Current output (Not this output, it displays 0.0000)
- 12.0017H: 0.0000 (This address is reserved by system and unrelated to the instrument data displays on the interface.)
- 13.0019H: Gauge temperature
- 14.001BH: Exceed to limited cumulative flow rate (When close the Protocol measurement, it displays 0.0000)
- 15.001DH: Total power outage time. (When the system clock is off, it displays 0.0000)
- 16.001FH: menu modification times

(4) Data Address


When the LCD screen displays the following data transmission information: NULL: transmission data 0

ERROR: transmission data -1234


OVERRUN: transmission data -8888

Appendix 7:Electrical Wiring

DB3

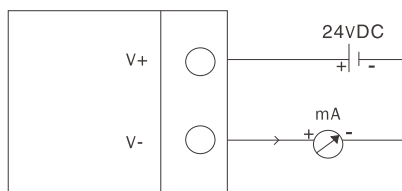


Current Output=Two Wire Connention

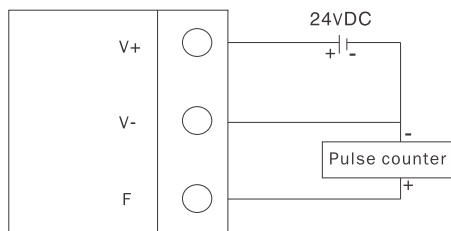


Frequency Output


DB4

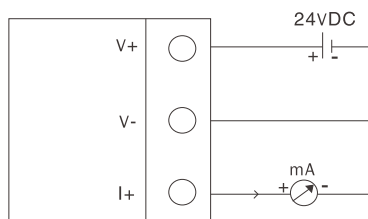

Current Output=Three Wire Connention

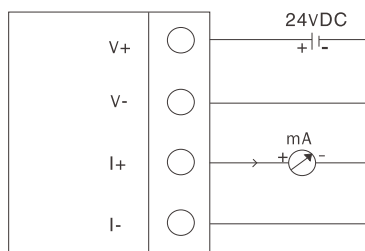


Current Output=Four Wire Connention

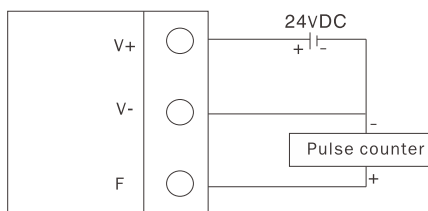


Frequency Output

Remote type wiring

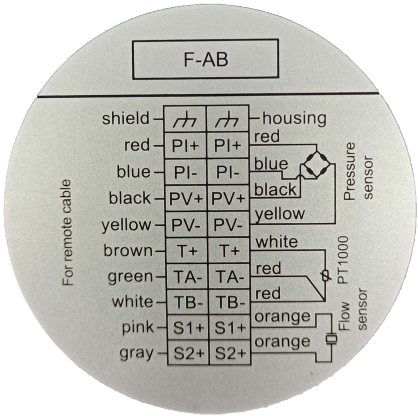

Sensor wiring

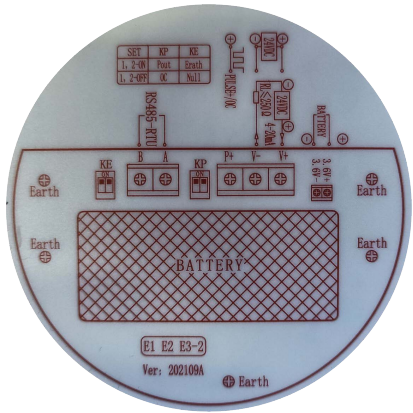

Converter wiring

KLINGER Danmark A/S
Nyager 12-14
DK-2605 Brøndby
Denmark
Phone +45 4364 6611